
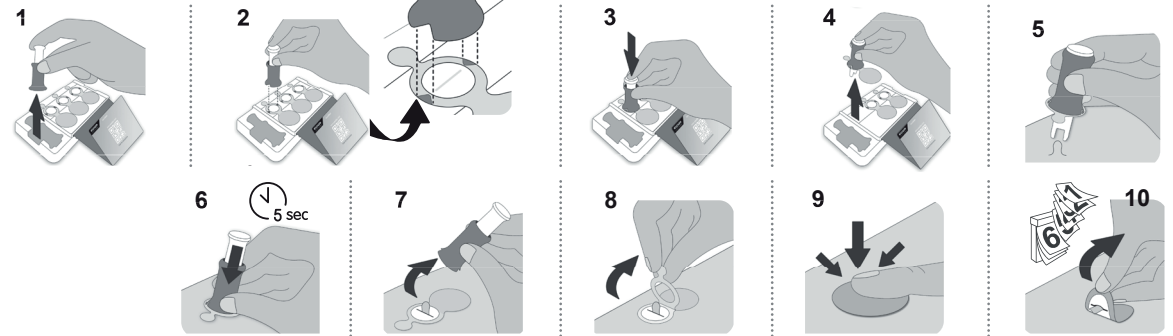


excilor®

SKINTAG TREATMENT

Watch the
VIDEO
INSTRUCTIONS

www.excilor.com

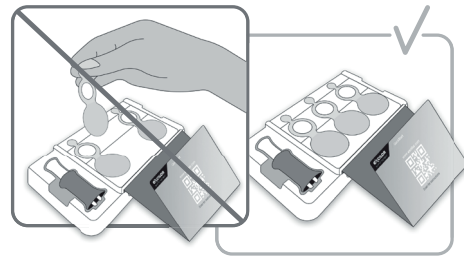

EN

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a medical device indicated for the removal of skin tags.

Read this instruction carefully before use.

SKIN TAGS

Skin tags are very common and harmless small, soft skin growths, 1-5 mm in diameter and 2-10 mm in height. They tend to occur on the neck, armpits, groin folds, eyelids, and under breasts. Skin tags can be irritating, bothersome and cosmetically embarrassing.

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a self-care device for the easy, safe, and painless removal of skin tags. When in place, the Excilor® Skintag Treatment device stops the flow of blood to the skin tag by way of ligation. The skin tag then gradually withers away in a safe way, with negligible risk of scarring and no pain. The skin tag must be max 3 mm in diameter at the base and max 5 mm in height. This Excilor® Skintag Treatment package contains an applicator and 3 skin tag devices, each one for the removal of one skin tag.

CAUTION

This product must be handled carefully and in accordance with the instructions for use.

Do not use Excilor® Skintag Treatment for removal of skin tags on the eyelids or near the eye, if the skin tag is not flesh coloured, does not fit within the diameter of the applicator (the skin tag must be max. 3mm in diameter at the base and max 5 mm in height) or is bleeding.

Consult your doctor, prior to use, if you have a history of skin cancer, have Hemophilia or if the skin tag shows signs of skin disease or infection.

Note that the skin tag device might not stay in place in groin or skin folds. Note that the withered skin tag will be necrotic after a few days. This is normal as the device will stop the flow of blood to the skin tag.

If you are in any doubt about whether the condition in question is in fact a skin tag, you should contact your doctor before initiating self-treatment. Do not use Excilor® Skintag Treatment if you are allergic to one or more of its ingredients/materials. For external use only. Keep out of reach and sight of children. Do not use under the age of 18 years. Do not use if the device is damaged.

Excilor® Skintag Treatment is safe to use during pregnancy and when breastfeeding.

HOW TO USE Excilor® Skintag Treatment

The Excilor® Skintag Treatment device consists of this instruction for use as well as:

- 1 applicator
- 3 discs on a blister carrier on a base

Clean the area around the skin tag with a washcloth and warm water. A mild soap can be used. However, avoid soaps and cleansers with oils, as well as impregnated wipes, since residue can prevent the plaster from sticking to the skin. Dry the area around the skin tag carefully.

Remove the applicator unit from the packaging as shown in figure 1. Hold the applicator as shown in figures 2.

Align the 2 indents of the blue part of the applicator base, with the 2 arrows printed on the plaster (enlarged view of figure 2).

Push down the white top so the applicator pushes through the center of the device (see figure 3), until it cannot be pushed further.

Pull back the applicator to remove the device from the blister carrier (figure 4). Place the device over the base of the skin tag (figure 5) with one leg of the applicator on each side of the skin tag. Then apply the device on the skin by pressing down the blue part of the applicator (figure 6). Press down and hold for a minimum of 5 seconds.

The device will automatically be locked in place on the skin tag. Lift the applicator away (figure 7).

Remove the paper liner by pulling the flap as indicated. (figure 8). Press the surface of the plaster cover with a finger to ensure that the adhesive sticks well to the skin (figure 9) and leave in place for 6 days (figure 10).

Do not scratch, rub or pick the plaster. Showering can take place, however, do not soak the area in water and do not go swimming.

Avoid soap, shampoo, hair products, body lotion, cream and oily substances on the area, as it can cause the plaster to loose prematurely.

For further instructions please find the online video on www.excilor.com or on YouTube or by scanning the QR-code.

WHAT TO EXPECT WHEN REMOVING the Excilor® Skintag Treatment device

The Excilor® Skintag Treatment device is removed after 6 days. When removing the device, the withered skin tag is normally removed as well.

Should Excilor® Skintag Treatment device fall off during the recommended period of use, do not replace, but wait 10 days to see if the treatment was successful. A normal plaster can be placed over the skin tag during this period. If the treatment was not successful, apply a new Excilor® Skintag Treatment device on the skin tag and remove after 6 days.

SIDE EFFECTS

Excilor® Skintag Treatment has no known side effects. The skin tag will be removed without pain and negligible scarring. A slight sensation during treatment might be felt after a few days. Leave the device in place. Insignificant bleeding might occur upon removal of the device.

A tiny mark might appear on the skin, however, it will disappear after some time.

STORAGE

Store out of the reach of children. Store at 2-30°C, away from direct sunlight and in the original packaging. Do not use Excilor® Skintag Treatment after the expiry date.

This Excilor® Skintag Treatment product can be disposed of as household waste.

Unigroup ApS, Diplomvej 373, DK-2800 Lyngby, Denmark.

Excilor® Skintag Treatment is a registered trademark. Excilor® Skintag Treatment is patent protected.

Registration: Excilor® Skintag Treatment is classified and registered as a medical device, class I, in accordance with the Medical Device Directive 93/42/EEC.



Information updated: XX-2017.

INGREDIENTS

Carrier: Polyester and synthetic rubber / Disc: Polyoxymethylene (POM) / Cover: Polyester and Acrylat

EN

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a medical device indicated for the removal of skin tags.

Read this instruction carefully before use.

SKIN TAGS

Skin tags are very common and harmless small, soft skin growths, 1-5 mm in diameter and 2-10 mm in height. They tend to occur on the neck, armpits, groin folds, eyelids, and under breasts. Skin tags can be irritating, bothersome and cosmetically embarrassing.

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a self-care device for the easy, safe, and painless removal of skin tags. When in place, the Excilor® Skintag Treatment device stops the flow of blood to the skin tag by way of ligation. The skin tag then gradually withers away in a safe way, with negligible risk of scarring and no pain. The skin tag must be max 3 mm in diameter at the base and max 5 mm in height. This Excilor® Skintag Treatment package contains an applicator and 3 skin tag devices, each one for the removal of one skin tag.

CAUTION

This product must be handled carefully and in accordance with the instructions for use.

Do not use Excilor® Skintag Treatment for removal of skin tags on the eyelids or near the eye, if the skin tag is not flesh coloured, does not fit within the diameter of the applicator (the skin tag must be max. 3mm in diameter at the base and max 5 mm in height) or is bleeding.

Consult your doctor, prior to use, if you have a history of skin cancer, have Hemophilia or if the skin tag shows signs of skin disease or infection.

Note that the skin tag device might not stay in place in groin or skin folds. Note that the withered skin tag will be necrotic after a few days. This is normal as the device will stop the flow of blood to the skin tag.

If you are in any doubt about whether the condition in question is in fact a skin tag, you should contact your doctor before initiating self-treatment. Do not use Excilor® Skintag Treatment if you are allergic to one or more of its ingredients/materials. For external use only. Keep out of reach and sight of children. Do not use under the age of 18 years. Do not use if the device is damaged.

Excilor® Skintag Treatment is safe to use during pregnancy and when breastfeeding.

HOW TO USE Excilor® Skintag Treatment

The Excilor® Skintag Treatment device consists of this instruction for use as well as:

- 1 applicator
- 3 discs on a blister carrier on a base

Clean the area around the skin tag with a washcloth and warm water. A mild soap can be used. However, avoid soaps and cleansers with oils, as well as impregnated wipes, since residue can prevent the plaster from sticking to the skin. Dry the area around the skin tag carefully.

Remove the applicator unit from the packaging as shown in figure 1. Hold the applicator as shown in figures 2.

Align the 2 indents of the blue part of the applicator base, with the 2 arrows printed on the plaster (enlarged view of figure 2).

Push down the white top so the applicator pushes through the center of the device (see figure 3), until it cannot be pushed further.

Pull back the applicator to remove the device from the blister carrier (figure 4). Place the device over the base of the skin tag (figure 5) with one leg of the applicator on each side of the skin tag. Then apply the device on the skin by pressing down the blue part of the applicator (figure 6). Press down and hold for a minimum of 5 seconds.

The device will automatically be locked in place on the skin tag. Lift the applicator away (figure 7).

Remove the paper liner by pulling the flap as indicated. (figure 8). Press the surface of the plaster cover with a finger to ensure that the adhesive sticks well to the skin (figure 9) and leave in place for 6 days (figure 10).

Do not scratch, rub or pick the plaster. Showering can take place, however, do not soak the area in water and do not go swimming.

Avoid soap, shampoo, hair products, body lotion, cream and oily substances on the area, as it can cause the plaster to loose prematurely.

For further instructions please find the online video on www.excilor.com or on YouTube or by scanning the QR-code.

WHAT TO EXPECT WHEN REMOVING the Excilor® Skintag Treatment device

The Excilor® Skintag Treatment device is removed after 6 days. When removing the device, the withered skin tag is normally removed as well.

Should Excilor® Skintag Treatment device fall off during the recommended period of use, do not replace, but wait 10 days to see if the treatment was successful. A normal plaster can be placed over the skin tag during this period. If the treatment was not successful, apply a new Excilor® Skintag Treatment device on the skin tag and remove after 6 days.

SIDE EFFECTS

Excilor® Skintag Treatment has no known side effects. The skin tag will be removed without pain and negligible scarring. A slight sensation during treatment might be felt after a few days. Leave the device in place. Insignificant bleeding might occur upon removal of the device.

A tiny mark might appear on the skin, however, it will disappear after some time.

STORAGE

Store out of the reach of children. Store at 2-30°C, away from direct sunlight and in the original packaging. Do not use Excilor® Skintag Treatment after the expiry date.

This Excilor® Skintag Treatment product can be disposed of as household waste.

Unigroup ApS, Diplomvej 373, DK-2800 Lyngby, Denmark.

Excilor® Skintag Treatment is a registered trademark. Excilor® Skintag Treatment is patent protected.

Registration: Excilor® Skintag Treatment is classified and registered as a medical device, class I, in accordance with the Medical Device Directive 93/42/EEC.



Information updated: XX-2017.

INGREDIENTS



Carrier: Polyester and synthetic rubber / Disc: Polyoxymethylene (POM) / Cover: Polyester and Acrylat

excilor®

SKINTAG TREATMENT

Watch the
VIDEO
INSTRUCTIONS

www.excilor.com

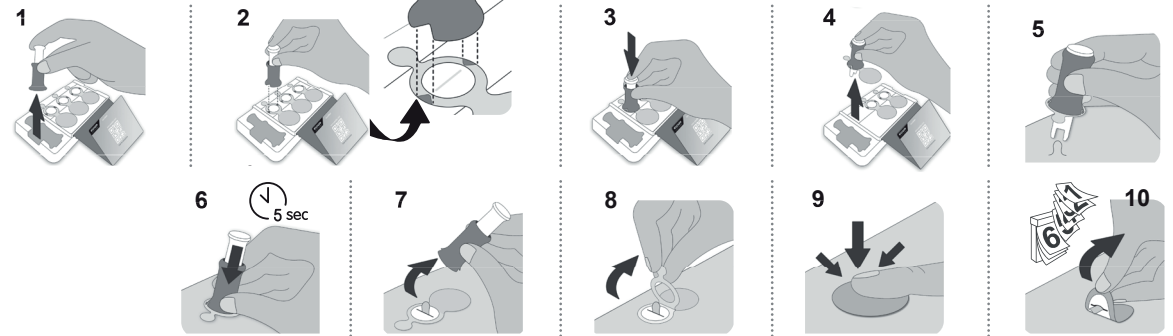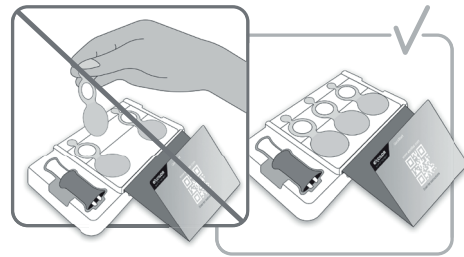

EN

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a medical device indicated for the removal of skin tags.

Read this instruction carefully before use.

SKIN TAGS

Skin tags are very common and harmless small, soft skin growths, 1-5 mm in diameter and 2-10 mm in height. They tend to occur on the neck, armpits, groin folds, eyelids, and under breasts. Skin tags can be irritating, bothersome and cosmetically embarrassing.

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a self-care device for the easy, safe, and painless removal of skin tags. When in place, the Excilor® Skintag Treatment device stops the flow of blood to the skin tag by way of ligation. The skin tag then gradually withers away in a safe way, with negligible risk of scarring and no pain. The skin tag must be max 3 mm in diameter at the base and max 5 mm in height. This Excilor® Skintag Treatment package contains an applicator and 3 skin tag devices, each one for the removal of one skin tag.

CAUTION

This product must be handled carefully and in accordance with the instructions for use.

Do not use Excilor® Skintag Treatment for removal of skin tags on the eyelids or near the eye, if the skin tag is not flesh coloured, does not fit within the diameter of the applicator (the skin tag must be max. 3mm in diameter at the base and max 5 mm in height) or is bleeding.

Consult your doctor, prior to use, if you have a history of skin cancer, have Hemophilia or if the skin tag shows signs of skin disease or infection.

Note that the skin tag device might not stay in place in groin or skin folds. Note that the withered skin tag will be necrotic after a few days. This is normal as the device will stop the flow of blood to the skin tag.

If you are in any doubt about whether the condition in question is in fact a skin tag, you should contact your doctor before initiating self-treatment. Do not use Excilor® Skintag Treatment if you are allergic to one or more of its ingredients/materials. For external use only. Keep out of reach and sight of children. Do not use under the age of 18 years. Do not use if the device is damaged.

Excilor® Skintag Treatment is safe to use during pregnancy and when breastfeeding.

HOW TO USE Excilor® Skintag Treatment

The Excilor® Skintag Treatment device consists of this instruction for use as well as:

- 1 applicator
- 3 discs on a blister carrier on a base

Clean the area around the skin tag with a washcloth and warm water. A mild soap can be used. However, avoid soaps and cleansers with oils, as well as impregnated wipes, since residue can prevent the plaster from sticking to the skin. Dry the area around the skin tag carefully.

Remove the applicator unit from the packaging as shown in figure 1. Hold the applicator as shown in figures 2.

Align the 2 indents of the blue part of the applicator base, with the 2 arrows printed on the plaster (enlarged view of figure 2).

Push down the white top so the applicator pushes through the center of the device (see figure 3), until it cannot be pushed further.

Pull back the applicator to remove the device from the blister carrier (figure 4). Place the device over the base of the skin tag (figure 5) with one leg of the applicator on each side of the skin tag. Then apply the device on the skin by pressing down the blue part of the applicator (figure 6). Press down and hold for a minimum of 5 seconds.

The device will automatically be locked in place on the skin tag. Lift the applicator away (figure 7).

Remove the paper liner by pulling the flap as indicated. (figure 8). Press the surface of the plaster cover with a finger to ensure that the adhesive sticks well to the skin (figure 9) and leave in place for 6 days (figure 10).

Do not scratch, rub or pick the plaster. Showering can take place, however, do not soak the area in water and do not go swimming.

Avoid soap, shampoo, hair products, body lotion, cream and oily substances on the area, as it can cause the plaster to loose prematurely.

For further instructions please find the online video on www.excilor.com or on YouTube or by scanning the QR-code.

WHAT TO EXPECT WHEN REMOVING the Excilor® Skintag Treatment device

The Excilor® Skintag Treatment device is removed after 6 days. When removing the device, the withered skin tag is normally removed as well.

Should Excilor® Skintag Treatment device fall off during the recommended period of use, do not replace, but wait 10 days to see if the treatment was successful. A normal plaster can be placed over the skin tag during this period. If the treatment was not successful, apply a new Excilor® Skintag Treatment device on the skin tag and remove after 6 days.

SIDE EFFECTS

Excilor® Skintag Treatment has no known side effects. The skin tag will be removed without pain and negligible scarring. A slight sensation during treatment might be felt after a few days. Leave the device in place. Insignificant bleeding might occur upon removal of the device. A tiny mark might appear on the skin, however, it will disappear after some time.

STORAGE

Store out of the reach of children. Store at 2-30°C, away from direct sunlight and in the original packaging. Do not use Excilor® Skintag Treatment after the expiry date.

This Excilor® Skintag Treatment product can be disposed of as household waste.

Unigroup ApS, Diplomvej 373, DK-2800 Lyngby, Denmark.

Excilor® Skintag Treatment is a registered trademark. Excilor® Skintag Treatment is patent protected.

Registration: Excilor® Skintag Treatment is classified and registered as a medical device, class I, in accordance with the Medical Device Directive 93/42/EEC.



Information updated: XX-2017.

INGREDIENTS

Carrier: Polyester and synthetic rubber / Disc: Polyoxymethylene (POM) / Cover: Polyester and Acrylat

EN

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a medical device indicated for the removal of skin tags.

Read this instruction carefully before use.

SKIN TAGS

Skin tags are very common and harmless small, soft skin growths, 1-5 mm in diameter and 2-10 mm in height. They tend to occur on the neck, armpits, groin folds, eyelids, and under breasts. Skin tags can be irritating, bothersome and cosmetically embarrassing.

Excilor® Skintag Treatment

Excilor® Skintag Treatment is a self-care device for the easy, safe, and painless removal of skin tags. When in place, the Excilor® Skintag Treatment device stops the flow of blood to the skin tag by way of ligation. The skin tag then gradually withers away in a safe way, with negligible risk of scarring and no pain. The skin tag must be max 3 mm in diameter at the base and max 5 mm in height. This Excilor® Skintag Treatment package contains an applicator and 3 skin tag devices, each one for the removal of one skin tag.

CAUTION

This product must be handled carefully and in accordance with the instructions for use.

Do not use Excilor® Skintag Treatment for removal of skin tags on the eyelids or near the eye, if the skin tag is not flesh coloured, does not fit within the diameter of the applicator (the skin tag must be max. 3mm in diameter at the base and max 5 mm in height) or is bleeding.

Consult your doctor, prior to use, if you have a history of skin cancer, have Hemophilia or if the skin tag shows signs of skin disease or infection.

Note that the skin tag device might not stay in place in groin or skin folds. Note that the withered skin tag will be necrotic after a few days. This is normal as the device will stop the flow of blood to the skin tag.

If you are in any doubt about whether the condition in question is in fact a skin tag, you should contact your doctor before initiating self-treatment. Do not use Excilor® Skintag Treatment if you are allergic to one or more of its ingredients/materials. For external use only. Keep out of reach and sight of children. Do not use under the age of 18 years. Do not use if the device is damaged.

Excilor® Skintag Treatment is safe to use during pregnancy and when breastfeeding.

HOW TO USE Excilor® Skintag Treatment

The Excilor® Skintag Treatment device consists of this instruction for use as well as:

- 1 applicator
- 3 discs on a blister carrier on a base

Clean the area around the skin tag with a washcloth and warm water. A mild soap can be used. However, avoid soaps and cleansers with oils, as well as impregnated wipes, since residue can prevent the plaster from sticking to the skin. Dry the area around the skin tag carefully.

Remove the applicator unit from the packaging as shown in figure 1. Hold the applicator as shown in figures 2.

Align the 2 indents of the blue part of the applicator base, with the 2 arrows printed on the plaster (enlarged view of figure 2).

Push down the white top so the applicator pushes through the center of the device (see figure 3), until it cannot be pushed further.

Pull back the applicator to remove the device from the blister carrier (figure 4). Place the device over the base of the skin tag (figure 5) with one leg of the applicator on each side of the skin tag. Then apply the device on the skin by pressing down the blue part of the applicator (figure 6). Press down and hold for a minimum of 5 seconds.

The device will automatically be locked in place on the skin tag. Lift the applicator away (figure 7).

Remove the paper liner by pulling the flap as indicated. (figure 8). Press the surface of the plaster cover with a finger to ensure that the adhesive sticks well to the skin (figure 9) and leave in place for 6 days (figure 10).

Do not scratch, rub or pick the plaster. Showering can take place, however, do not soak the area in water and do not go swimming.

Avoid soap, shampoo, hair products, body lotion, cream and oily substances on the area, as it can cause the plaster to loose prematurely.

For further instructions please find the online video on www.excilor.com or on YouTube or by scanning the QR-code.

WHAT TO EXPECT WHEN REMOVING the Excilor® Skintag Treatment device

The Excilor® Skintag Treatment device is removed after 6 days. When removing the device, the withered skin tag is normally removed as well.

Should Excilor® Skintag Treatment device fall off during the recommended period of use, do not replace, but wait 10 days to see if the treatment was successful. A normal plaster can be placed over the skin tag during this period. If the treatment was not successful, apply a new Excilor® Skintag Treatment device on the skin tag and remove after 6 days.

SIDE EFFECTS

Excilor® Skintag Treatment has no known side effects. The skin tag will be removed without pain and negligible scarring. A slight sensation during treatment might be felt after a few days. Leave the device in place. Insignificant bleeding might occur upon removal of the device. A tiny mark might appear on the skin, however, it will disappear after some time.

STORAGE

Store out of the reach of children. Store at 2-30°C, away from direct sunlight and in the original packaging. Do not use Excilor® Skintag Treatment after the expiry date.

This Excilor® Skintag Treatment product can be disposed of as household waste.

Unigroup ApS, Diplomvej 373, DK-2800 Lyngby, Denmark.

Excilor® Skintag Treatment is a registered trademark. Excilor® Skintag Treatment is patent protected.

Registration: Excilor® Skintag Treatment is classified and registered as a medical device, class I, in accordance with the Medical Device Directive 93/42/EEC.



Information updated: XX-2017.

INGREDIENTS

Carrier: Polyester and synthetic rubber / Disc: Polyoxymethylene (POM) / Cover: Polyester and Acrylat